


There's no longer just
one source
for single click
manufacturer
IFU documents

BLUE  i f u

 **The Joint Commission**

Percentage of Surveyed Hospitals Noncompliant with IC.02.02.01

(Standard requires facility to reduce the risk of infections associated with medical equip., devices and supplies)

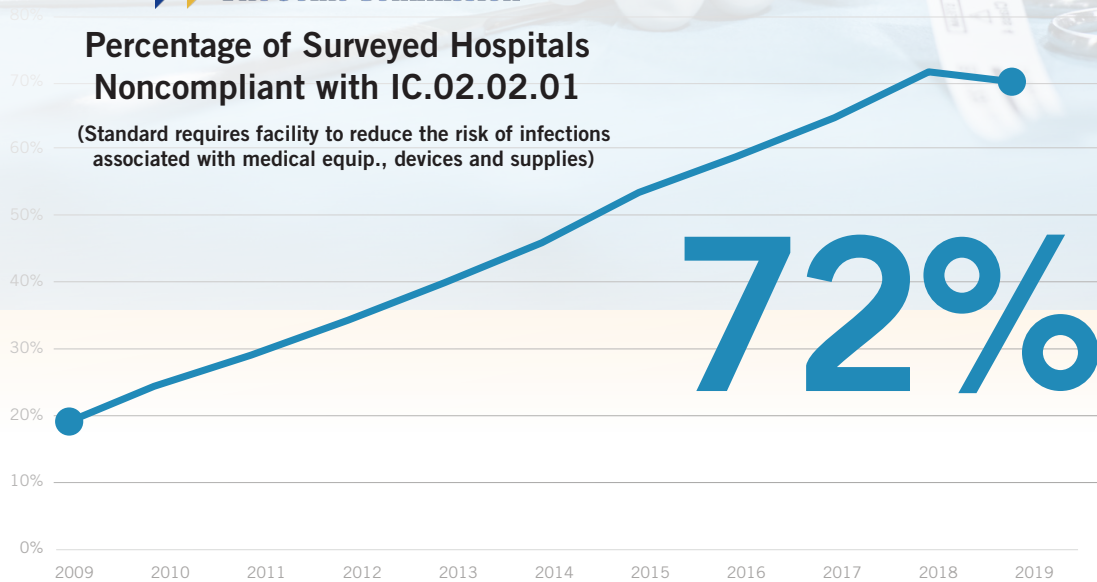

72%

HEALTHCARE FACILITIES MUST COMPLY WITH EVOLVING OPERATIONAL MANDATES FROM THE JOINT COMMISSION, AAMI, AORN, CMS, AND OTHER REGULATORY AGENCIES.

Immediate single-click access to see the required step-by-step instructions of validated manufacturer IFUs is critical. Failure to correctly follow the IFU puts patients, surgical staff and sterile processing professionals at risk. It also carries financial, legal, and reputational risk to the business.

BLUE  i f u **can empower your team to**

- Enhance patient & staff safety
- Minimize the risk of SSIs
- Lower re-admissions
- Reduce errors in IFU decontamination
- Improve IFU sterilization
- Enhance SPD performance

Instruments, Dental, Impants and more, BLUEifu is offered at a 15–25% savings over the other source!

The BLUEifu platform provides instant cloud-based access to IFUs from leading global manufacturers. BLUEifu helps your team combat the daily errors performed in EVERY sterilization department across the country.

From the makers of the leading IFU sterilization intelligence software

 **PETRISS**
STERILIZATION INTELLIGENCE

Pursue 100% Compliance

BLUE  ifu

Cloud-based platform is constantly updated when new validated IFUs are issued. Subscribing to BLUEifu is easy, seamless and flexible.

POWERFUL OUTCOMES

BLUE  fin

Take your IFU compliance to the next level with the BLUEfin platform, which offers real-time guidance on IFU instructions with videos that clarify complex steps, built-in timers, and automatic documentation that demonstrates compliance.

The BLUEfin platform automatically creates real-time guidance and transparent documentation to prove compliance with TJC, AAMI, AORN, CMS and other regulatory expectations. Any non-compliant behavior is flagged for additional training and remediation.

“It is important to understand that each patient care item has its own IFUs for cleaning and disinfection. Failure to follow such instructions or misuse creates significant risk to safe, quality care.”

— The Joint Commission’s Expectations for IFUs, 2021

Non-compliance rate with IC.02.02.01, for proper surgical instrument sterilization

72%


 **PETRISS**
STERILIZATION INTELLIGENCE

\$14,400



Average cost for a hospital readmission, across all diagnoses

\$41.3 BILLION

 Associated cost of hospital readmissions, per year



 = 100,000 PEOPLE

4.28 MILLION

Number of people readmitted to the hospital within 30 days, per year

THE 30-DAY HOSPITAL READMISSION RATE, ACROSS ALL DIAGNOSES

13.9%



3 out of 4 Immediate THREAT TO LIFE

declarations by TJC are related to improperly sterilized equipment

2,599

Hospitals received readmission penalties in fiscal 2019



Sources: The Joint Commission, the Agency for Healthcare Research and Quality, and the Hospital Readmissions Reduction Program.

www.petrissinc.com

sales@petrissinc.com | 770-853-5066

505 COMMERCE PARK DRIVE, SUITE F, MARIETTA, GA 30060